



低压型气密检漏仪 Low-Pressure Air Leak Tester


FL-295D 系列 Series

- 调压阀稳压精度可达0.1kPa (UL可达0.01kPa)
- 泄漏单位Pa, mL/min, mmH₂O, L/h可选
- 被测物容积可自动读取或手动输入
- 500组测试数据存储器, 最新99组数据查看
- 最多16组测试通道
- 9999个数据统计 (OK、NG、P. NG个数)
- 通讯接口支持软件升级



- Regulator Accuracy Can Reach 0.1kPa (UL Can Reach 0.01 kPa)
- Leakage Units: Pa, mL/min, mmH₂O, L/h
- Work Volume Can be Loaded Automatically or Inputted Manually
- Can Memory 500 Groups Testing Data, View Latest 99 Groups Data
- Maximum 16 Groups Testing Channels
- 9999 Data Statistics (OK,NG,P. NG)
- Support Communication Port Software Upgrading

外形尺寸
Dimensions
(mm)

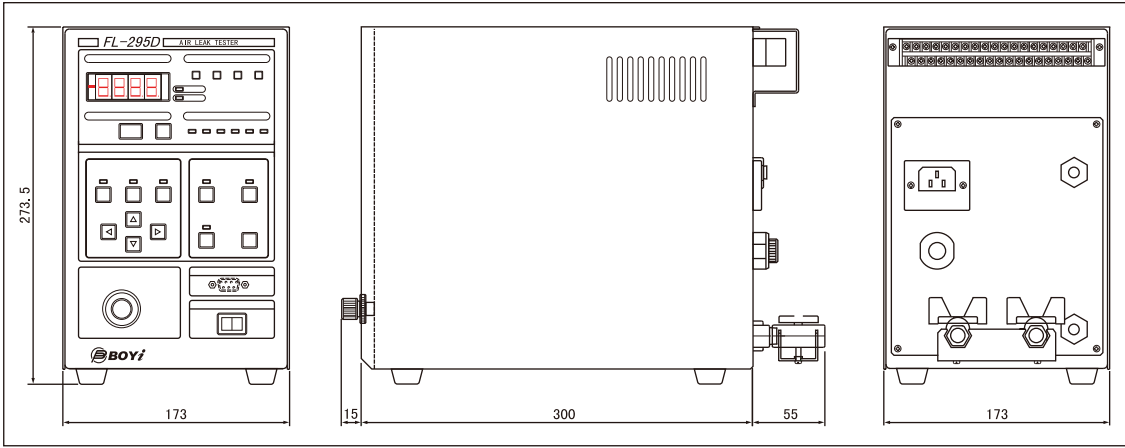

选型 FL-295D ①-②-③-④ Ordering Information

① 型号 Mode

记号 Denotation	测量范围 Measuring Range (mL/min)	被测容积范围 Work Volume (mL)	测试压范围 Test Pressure (kPa)
UL	0.010~2.000	5~200	0.50~10.00
S	0.010~2.000	5~200	3.0~50.0※
L	0.25~9.99	100~1000	3.0~50.0※

※ 测试压力超出范围需特制 ※ Customized product can be provided if test pressure is out of range.

② 选购品 Options

记号 Denotation	含义 Descriptions
P	打印机 Printer Output
R	RS-232C输出 RS-232C Output

③ UL用调压装置 Pressure Adjustment Equipment for Mode UL

记号 Denotation	含义 Descriptions
FR11	调压阀 (0.50~10.00kPa用) Regulator
PC-295	压力切换盒 (0.50~20.00kPa用) Pressure Switching Box
N	无调压装置 Without voltage regulator

④ 前级减压阀 Preceding stage pressure reducing valve

记号 Denotation	含义 Descriptions
FR31	减压阀 (10~100kPa用) Pressure reducing valve (10~100kPa use)
N	无调压装置 Without voltage regulator

技术指标 Specifications

参数 Parameters

测 试 方 式 Test Method	差压比较方式 Differential Pressure Measurement Method		
压 力 传 感 器 Pressure Sensor	差压传感器 Differential Pressure Sensor		F.S.±1000Pa 精度:±1%F.S.
	直压传感器	S、L	F.S. 50kPa 精度:±1%F.S.
	Gauge Pressure Sensor	UL	F.S. 20kPa 精度:±1%F.S.
时 间 设 置 Time Settings	CHG (充气 Charge)	0.2~999.9	单 位 Unit 秒 Second
	BAL (平衡 Balance)	0.2~999.9	
	DET (检测 Detect)	0.2~99.9	
	EXH (排气 Exhaust)	1~999.9	
测定精度 Measuring Accuracy	100ml 标准被测物1ml/min的泄漏测试下，测定误差在±5%以内 Measuring deviation less than ±5%, on the condition that standard work is 100ml, leak rate is 1ml/min in testing.		
组 别 设 定 内 容 Group Setting Function	CHG、BAL、DET、EXH、±NG、P.NG、校正值 Calibrating Value		
辅 助 功 能 Auxiliary Function	BUBL (气泡测试 Bubble Test) CAL (校正 Calibration)		
显 示 Display	S/UL 系列为4位数字显示，L 系列为3位数字显示 S/UL Series: 4 Digits Display L Series: 3 Digits Display		
输 入 输 出 I/O	外部输入输出端子 (38 针) External I/O Terminal (38 pin)		
	输出选择: Output Options	* 打印机 * RS-232C (9 针)	Printer RS-232C (9 Pin)

系统组成 System Structure	检漏仪内部带有控制驱动器, 只要配备了夹具、气缸、电磁阀及开关后, 即可经济、方便地组成整个检测系统。 There is a control drive in the leak tester, as long as it is equipped jig, cylinder and solenoid valve, they can be consisted a whole testing system in convenient and economical ways.	
温度范围 Temperature Requirement	0~40℃	
湿度范围 Humidity Requirement	35~85%RH (无结露现象 No Dew)	
电源电压 Power Supply	AC100~240V (50/60Hz)	
功率 Power Consumption	≤50W	
重量 Weight	8kg	
气源要求 Air Supply Specifications	洁净、干燥、压力稳定的空气 Clean, Dry, Stable Air	
	建议条件 Optimal	大气压露点-17℃以下, 油含量0.1mgf/Nm³ 以下, 固体杂质0.01μm 以下 Below Atmospheric Dew Point-17℃, Oil Content below 0.1mgf/Nm³, Solid Impurity Smaller than 0.01μm
一次压力 Inlet Pressure	100kPa	

主要产品 ● 气密检漏仪 ● 数字压力表 ● 流量计 ● 自动压力、流量控制器 ● 密封性能检测专用设备

代理经销商



公司·工厂: 天津开发区第九大街80号丰华工业园7号厂区 邮编: 300457
电话: (86)22-59810966 传真: (86)22-59810963
营销中心: 北京市丰台区角门18号名流未来大厦801-805室 邮编: 100068
电话: (86)10-87582461 传真: (86)10-87582462
网址: www.boyiqd.com 邮箱: sales@boyiqd.com



扫一扫, 查看
办事处地址

公司在广州、顺德、杭州、台州、宁波、上海、苏州、武汉、重庆、西安、济南、沈阳设有分支机构。

C-BY-000295D-X-04
Printed in China